

Dive Talk Go
www.DiveTalkGO.com
info@divetalkgo.com



DIVE TALK GO MANUAL

READ THE MANUAL!!!!

IN ORDER TO FULLY UNDERSTAND YOUR NEW REBREATHER, THE COMPONENTS, HOW THEY WORK, HOW TO HANDLE AND TREAT THEM, YOU MUST READ THE MANUAL IN FULL, FOR YOUR REBREATHER.

THIS SHOULD BE DONE PRIOR TO DIVING OR SERVICING THIS UNIT!!! SPECIAL ATTENTION SHOULD BE PAID TO ALL NOTES &/OR WARNINGS; THEY MUST BE READ AND UNDERSTOOD!!!! FAILURE TO DO SO, MAY CAUSE SERIOUS INJURY OR DEATH!!!!

DO NOT MODIFY THE DIVE TALK GO REBREATHER. UNAUTHORIZED MODIFICATIONS COULD CAUSE SERIOUS INJURY OR DEATH!!!

YOU MUST BE A LEGAL ADULT IN THE AREA IN WHICH YOU LIVE IN ORDER TO PURCHASE AND DIVE A DIVE TALK GO REBREATHER.

- DO NOT USE THE REBREATHER WITHOUT FIRST SUCCESSFULLY COMPLETING A UNIT SPECIFIC TRAINING COURSE APPROVED BY DIVETALK.***
- REBREATHER DIVING IS PHYSICALLY AND MENTALLY DEMANDING. DO NOT USE THE REBREATHER UNLESS YOU ARE PHYSICALLY, MEDICALLY AND MENTALLY FIT TO UNDERTAKE THIS ACTIVITY PRIOR TO DIVING.***

As with all scuba diving equipment, your Dive Talk rebreather components should be serviced annually by a trained technician. For those diving frequently, servicing may be required more often.

ALL INFORMATION IN THIS MANUAL IS SUBJECT TO CHANGE.

**Please visit our website, www.DiveTalkGO.com
for updated manuals.**

THIS IS NOT A JOKE!!



Participation in rebreather diving can result in serious injury or death to you, the diver!

The warning on the Dive Talk Go rebreather is not a joke. Before beginning your dive, you must consider the risks involved. The DT Go consists of many parts. All of these components will eventually fail. Careful maintenance, assembly, and testing will not prevent this from happening. At best, it will delay the failure. The DT Go is not automatic in any way. It requires constant monitoring, a complete awareness of the potential problems likely to be encountered, and full knowledge of how to deal with whatever problems may occur. If you do not have adequate training, equipment, physical conditioning, and a proper mind-set, do not get in the water.

The diver, YOU, has the final responsibility for his or her own safety and actions while using this rebreather. All components of the DT Go must be in good working order and be properly assembled and tested to reduce the risk of failure. Regardless of the training and experience of the diver and the reliability of the rebreather the risk of serious injury and/or death can never be reduced to zero.

This manual is not a complete text on the maintenance and operation of the DT Go. The diver must complete a proper training course covering the maintenance, testing and operation of the rebreather before diving this equipment. The rebreather can malfunction while diving even when properly assembled and having passed all pre-dive tests. Only carrying adequate bailout gas and having the training and skills necessary to utilize the bailout system can reduce, but never eliminate, the risk of equipment failure.

TABLE OF CONTENTS

| | |
|---|---------|
| Introduction | Page 5 |
| Specifications | Page 6 |
| Parts List | Page 7 |
| Unpacking & Disassembly | Page 9 |
| 4 pin cable | Page 10 |
| Oxygen Sensors | Page 11 |
| Automatic Diluent Valve (ADV) | Page 14 |
| Oxygen Manual Add Valve/Metering Orifice | Page 15 |
| Oxygen First Stage Regulator & Flow Rates | Page 19 |
| Mouthpiece/DSV maintenance | Page 22 |
| Mouthpiece Test | Page 24 |
| Mouthpiece Servicing & Troubleshooting | Page 25 |
| Loop Hoses & Hose Stubs | Page 27 |
| Diluent Cylinder & Quick Connect System | Page 28 |
| Filling the Scrubber Canister | Page 30 |
| Counterlung Installation | Page 32 |
| Loop Hose & ADV Assembly | Page 34 |
| Positive & Negative Testing | Page 35 |
| Dive Computer & Calibration | Page 38 |
| Pre-dive Checklist | Page 42 |
| Troubleshooting - Exhaust Valve, ADV, & Work of Breathing | Page 46 |
| Warranty | Page 49 |
| CCR Diver Information Sheet | Page 50 |
| RESA Recommends | Page 52 |
| Dive Talk Evaluation Form - CCR Diver Level | |
| Dive Talk Minimum Training Standards - CCR Diver Level | |

Introducing, The Dive Talk GO

Operations Manual

The Dive Talk GO MCCR exemplifies unmatched convenience and performance, weighing just 10 lb/ 4.5 kg without the absorbent or cylinder, and approximately 18.2 lb/8.3 kg with absorbent. Its versatile chest mount design allows for seamless attachment to any BCD, catering to both recreational and technical divers.

From effortless packing in a carry-on suitcase to minimal space requirements on boat dives, the Dive Talk GO MCCR ensures unparalleled portability. With exceptional work of breathing and straightforward assembly, divers can relish extended 3-hour dives, making it their preferred choice. Its straightforward design and versatility make it stand out, offering comparable benefits to heavier and pricier units. Embrace the Dive Talk GO MCCR as the effortless, adaptable solution for both back mount and side mount preferences, fitting seamlessly onto any recreational BCD.

Specifications: DIVE TALK GO

- Weight of the unit completely assembled with a full scrubber canister is, 18.2lb/ 8.3kg.
- The weight of the unit without the cylinder and no absorbent is 10lb/4.5kg. This would be the weight of the system for flying without the cylinder.
- The length of the unit ready to dive is 14.5 inches/36.83 cm.
- The widest part of the unit is 12.5 inches/31.75 cm.
- PLEASE SEE OUR PARTS LIST ON THE NEXT PAGE FOR A FULL LIST OF WHAT IS INCLUDED AND WHAT IS NOT.
- It is a mechanical rebreather which adds O₂ continuously by a feed orifice and manually as needed.
- Compatible with Trimix.
- Work of breathing: 132 feet/ 40 meters is 1.07 J/L.
- Scrubber holds approximately 3.5 lb/1.59 kg of absorbent, depending on the brand. Divers must use 8-12 granule size.

***WARNING: The use of larger granules can cause channeling. This can cause serious injury or death!**

- The Dive Talk Go is a closed circuit rebreather designed for recreational diving to the depth of 132 feet (40 meters). Proper training, outside the basic DT Go rebreather course is required for any deep or technical diving. For some types of diving, extra gear must be carried or alternate gear configurations will be required. Ensure you have the proper training, gases and gear to conduct your planned dive.
- A bailout system is required for all dives. The bailout system should be appropriate for the dive that is planned. Dive Talk strongly recommends that a second stage regulator is attached to the bailout first stages, using a LP hose. Dive Talk does not recommend using quick connects on regulator hoses, which have a regulator attached.

Parts List

!

The Dive Talk Go body includes:

- Removable screen
- 6 scrubber tension springs
- Attached ADV with low pressure hose
- Attached oxygen MAV
- Left and right counterlungs
- Loop hoses
- DSV
- Blocked oxygen first stage, includes OPV and pressure gauge
- Attached back plate with quick connect
- Oxygen cylinder bracket

Display Options are priced extra:

- Shearwater Petrel decompression computer
- Shearwater NERD, 4 pin system

Not included:

- Diluent low pressure inflator hose
- Diluent bail out regulator
- Diluent bail out cylinder
- BCD
- 3 DT-SMB sensors




Unpacking & Disassembly

Congratulations! You have just received your Dive Talk Go! The first thing to do is ensure that all the parts you ordered, are included in the box. As you know, the DT Go can be shipped either as the BASIC unit or with various components added. Please see the previous parts page for a list of what is included with the BASIC kit, and what the optional extras are. Go through the box and ensure that everything that you ordered has arrived. Small items can be lost in bubble wrap so ensure that you look carefully in the packing material also. The package will also include a thumb drive which contains your manual.

The DT Go ships with all the O-rings installed and the unit is assembled. The following instructions are for disassembling the Go.

- The counterlungs will be in the box, but not attached to the unit. Take them out.
- The mouthpiece/DSV will be wrapped separately. Take it out of the box, and unwrap it.
- Lay the unit face-down, and undo the 3 stainless steel latches by pushing the lock lever, then lifting the latch.

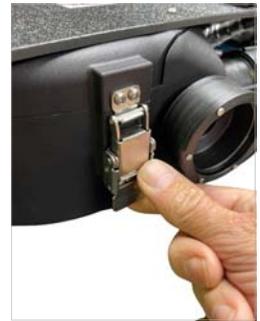

- Open the unit by pushing down on the ADV, and then pulling up on the inhale tower.



- Pull the top screen out.



The unit is now disassembled. Further sections of this manual will discuss assembly, scrubber packing, sensor installation & displays, and trouble shooting.

Four Pin Cable - Installation & Care

How to install a 4 pin cable:

The 4 pin cable can be installed or removed with a 15mm wrench. To ensure that the inner wires do not get twisted, after each turn (installing or removing) stop and straighten out the wires.



Having a 4 pin cable on a rebreather display system is a convenience that many divers enjoy. While a lot of maintenance is not required, some care is important in order to ensure that they operate properly.

The 4 pin port is watertight and any water that gets in to the port cannot harm your head, computer, or NERD. However, should sea water get inside the port or the ends of your linking cable, flush them with fresh water as soon as possible afterwards then leave them to dry completely BEFORE refitting the cap.

Regular maintenance should include:

1. Inspect the connectors and look for any signs of corrosion; parts will start to turn green.
2. If you see green/corrosion, rinse the connectors briefly with white vinegar and use a fine toothbrush to remove the build-up. Rinse well and let dry completely. Coat with a protective product such as Deoxit Gold.
3. Keep the 4 pins lubricated by applying a SMALL amount of Dielectric grease such as Dow Corning 111 on the metal end of the cable end that slides into the 4 pin connector. This will serve to improve the seal and make the connection more reliable. Always use a strain relief to keep the cables connected, while in use.

Remember, the cleanliness of the contacts is essential to the integrity of the link. Following these simple steps will ensure that your system works properly. Look after your cable and connectors and they will look after you.

Oxygen Sensors

The DT Go uses 3 oxygen sensors. The part number is, DT-SMB.

The sensors are simple to install, and use the SMB connection system. First, secure each SMB connector to the back of each sensor.



Next, put each sensor on the cradle and stretch the O-ring over it. This will hold the sensor in place.



***WARNING: The DT Go uses the Shearwater computers. As with all electronics, these components must be treated with care and respect. This includes taking care to not drop, bang, or roughly handle them. Also, do not leave these components in a hot environment, such as a car or direct sunlight. The heat &/or sun, can and will damage any electronic components.**

***WARNING: Do not mix sensor brands in your rebreather! There are various sensor brands available in the market place. If you mix brand "A" with brand "B", they will not work properly. As the response times are different for each brand, most electronics will not calibrate properly. If they do calibrate, they may not work correctly while diving as the different response times could cause an error reading.**

The DT Go uses the rebreather sensor, DT-SMB. The DT Go does not include the sensors. Many of our dealers stock the DT-SMB sensor and they are available directly from them. Should you wish to order them with your unit, please let us know your wish to add this product.

Prior to installing them, it is best to open the bags and let them sit for at least 24 hours prior to calibration as they need to go through a "wake up" period. Ideally, open the bags about a week prior to use, if possible. New sensors will read low when first installed and will creep up slightly over the course of a week or so. After that, they seem to be stable for months on end.

Don't waste time calibrating the sensors if they are reading within a 1/2 percent. These sensors should be changed annually, sooner if they are damaged or abused. Oxygen sensors work on the same basis as a battery. The more that they are used, the more often they will need to be replaced.

An easy way to remember your sensors anniversary date is to write the date on the top of the sensor. The DT-SMB sensors are safe to dive if the millivolt reading is between 9 and 13, AND they must be calibrated in oxygen. The Shearwater computers will read the millivolts of the sensors or a volt meter can be purchased at your local hardware or electronics store.

***WARNING: It is extremely important that the sensors millivolt readings are in the correct range, and that they can be calibrated in oxygen, and verified with air. If even just one of these 3 items doesn't comply, DO NOT DIVE!!!! Failure to ensure that the sensors are working properly, can result in serious injury or death!!!**

***WARNING: On the following pages are the calibration instructions for the displays systems. It is essential that the calibration procedures are followed properly. Also, DT Go divers must take the time to thoroughly read the Shearwater manuals. Divers must read and understand them, especially the sections on calibration. Failure to do so can cause injury or death!!**

***WARNING: It is important that the display cables are properly wired. Failure to do so, may cause serious injury or death! Ensure that the O-rings are in good condition, that the area is clean and the components are not damaged. Lastly, if the wires are pinched under the plate, the scrubber head will not be water tight. Water damage in this area will ruin the sensors and/or the electronics. If the wires do get pinched, inspect them for damage!!**

When you open up your new DT-SMB sensors, they will have a millivolt reading between 9 and 13 millivolts, in air. As long as they are in that range, they are safe to use. In 100% oxygen, at sea level the sensors should be between 40 and 60 millivolts.

***WARNING: You also need to ensure that they can be calibrated in Oxygen, and that they read correctly in air. This is very important. Even if a sensor is reading in the proper range, as it ages you may no longer be able to calibrate it properly. Sensors should not be used for more than 1 year.**

*****IF THIS HAPPENS, THE SENSOR MUST BE DISCARDED. FAILURE TO USE A PROPER SENSOR WILL CAUSE SERIOUS INJURY OR DEATH!!!!!!!!!!!!**

***Warning: Oxygen sensors are a fuel cell. As they age, they run lower on fuel, and will become voltage limited. They will read correctly in air, and calibrate in 100% oxygen, BUT as the partial pressure gets higher, they will no longer have the fuel to produce higher millivolts. Thus, they are VOLTAGE LIMITED, and will read incorrectly. THIS COULD CAUSE SERIOUS INJURY OR DEATH!!**

In diving applications the sensor will last 1 year, depending on how often you dive and how they are stored. Sensors should be allowed to dry out after your day of diving, especially if you are diving in a humid environment. This means that you need to leave the loop hoses or scrubber canister off overnight to allow air to circulate through the scrubber head. Leaving the unit sealed up will not allow the condensation to evaporate.

*****If the DT Go has moisture in the head from diving or from being in a humid environment, and it is then sealed up tight, the wires from the end of the display will start to corrode!!!! If this happens, whatever display or computer you are using, will not work properly!!!! It is extremely important that the head is allowed to dry out if the unit is to be sealed up. This means that after a dive trip, don't just drop the unit on your work bench and walk away from it!!! At the very least, drop the canister's off and let the head's dry. This will help keep your wires in good working order.**

Sea water on the sensors will probably cause them to fail.

As your sensors start to age you will notice that they are harder to calibrate, slower to react and will drift more after calibration.

Electrolyte, which is a gel like substance is inside the sensors. If you notice this substance leaking out of the sensors, do not touch it as it is caustic. Do not dive with a leaking sensor. The readings will be high!!!!

Automatic Diluent Valve (ADV)

AUTOMATIC DILUENT VALVE (ADV):

The ADV is located on the top of the gas addition scrubber head. The ADV will add diluent gas to your breathing loop after the loop volume has been reduced by either descending or “breathing down” the volume of oxygen. The diver will get the feeling that there is no more air in the loop to breath. All the diver needs to do is suck hard to trigger the ADV and it will feed him more gas. This is how a second stage regulator works.

The ADV has been setup “tight” enough so that it doesn’t add diluent without the diver being aware. But it adds enough gas so that a reasonable descent rate can be maintained. As you can see, there is an adjustment knob on the ADV regulator. It is very important that this knob is always tight and turned all the way in. As such, the diver’s must be aware of body position at all times and understand that a trim position will cause the ADV to activate more rapidly then other positions.

***WARNING: THE ADJUSTMENT KNOB ON THE ADV REGULATOR MUST ALWAYS BE TIGHT AND TURNED ALL THE WAY IN. ALSO, THE DIVER SHOULD BE AWARE THAT IN A HEAD-DOWN POSITION THE ADV MAY TRIGGER MORE RAPIDLY, CAUSING A RAPID ADDITION OF GAS. THIS WILL CAUSE BUOYANCY ISSUES WHICH MAY CAUSE THE DIVER TO HAVE AN UNCONTROLLED ASCENT, WHICH MAY LEAD TO INJURY OR DEATH!**

Anytime the ADV triggers you need to check your PPO2. you have either descended and compressed the gas in the loop or you have consumed enough oxygen to reduce the PPO2 significantly . This may also have caused you to lose buoyancy and descend.

The position of the diver will effect the ADV. If the diver is horizontal or face down, the ADV will trigger easily. If the diver is vertical, then it is more difficult to trigger. (A well fitting harness is important; this will greatly reduce the difficulties of being vertical in the water).



Adjustable ADV



Non-Adjustable ADV

Oxygen Manual Add Valve/Metering Orifice

The oxygen MAV, which is mounted to the unit, is the component that will add oxygen to your unit continuously and will also allow you to push a button to add gas as required.

The DT Go rebreather is mechanically controlled. The oxygen manual add valve houses a orifice which allows oxygen to flow into the loop at all times. In the event that more oxygen is required, the button on the O2 valve will need to be pushed. The difference between diving a DT Go rebreather manually and other rebreather's is that the constant flow of oxygen keeps our divers from getting too busy underwater. Diving other rebreather's manually means that the only way oxygen gets into the loop is by pushing the button.

What does this mean to the diver? It means that when you get to your maximum depth, you will adjust your PPO2 and then unless you are working hard or going up and down in the water column, you will only be pushing the button every 10 to 20 minutes. This depends also on where the constant flow has been set. If you find yourself pushing the button all the time, then you need to increase the flow. If you find that your oxygen is creeping up during normal diving activities, then you will want to decrease the flow.

***WARNING: WHEN YOU DO YOUR TRAINING COURSE, WITH THE HELP OF YOUR INSTRUCTOR, YOU WILL MONITOR THE FLOW RATE. IF YOU ARE CONSTANTLY PUSHING THE BUTTON, YOU WILL NEED TO INCREASE THE FLOW. IF YOUR OXYGEN IS CREEPING UP DURING NORMAL DIVING ACTIVITIES, YOU WILL NEED TO DECREASE THE FLOW. YOU MUST BE AWARE OF YOUR FLOW RATE AND UNDERSTAND HOW IT WORKS. FAILURE TO DO THIS, MAY CAUSE SERIOUS INJURY OR DEATH!**

The oxygen manual add valve on the DT Go should be serviced by a qualified technician annually.

***WARNING: THE OXYGEN MANUAL ADD VALVE MUST BE SERVICED BY A QUALIFIED TECHNICIAN ANNUALLY. FAILURE TO DO THIS, MAY CAUSE INJURY OR DEATH!**

Getting started and understanding the oxygen flow rate:

When you first receive your DT Go, a flow rate time test should be conducted. This is the best way to determine if your flow rate changes over time.

- With the DT Go fully assembled, secure a cylinder with more than 2000 psi of gas.
- Open the valve to pressurize the system.
- Close the valve, and watch the pressure gauge. The gauge should start bleeding down.
- Once the gauge is at 2000 psi/137.9 bar start a timer and note how long it takes for the system to bleed down to 1000 psi/68.9 bar. It should take approximately 50 to 60 seconds, depending on the configuration of the system, and other variables.




Once you have this information, write it down and keep it safe. It will be your reference later on when you double check your flow rate.

It should be noted that the rate of pressure drop during the flow rate test will vary (largely) depending on the length of the high-pressure hose and gauge that is installed on the first stage regulator. Changing the length of this hose, or removing it all together, will alter the flow rate time test.

Oxygen Add Valve Inner Components:

The oxygen manual add valve is for adding oxygen to the loop. The O-rings should be changed annually or if the flow rate changes. The inlet of the valve is protected by a 20 micron filter. This filter will NOT stop seawater from contaminating the orifice. All components in the oxygen add valve must be clean, oil free, with the O-rings lightly lubricated with oxygen compatible grease. The oxygen MAV is attached with 3 Phillips head screws. It can be removed to send in for service.

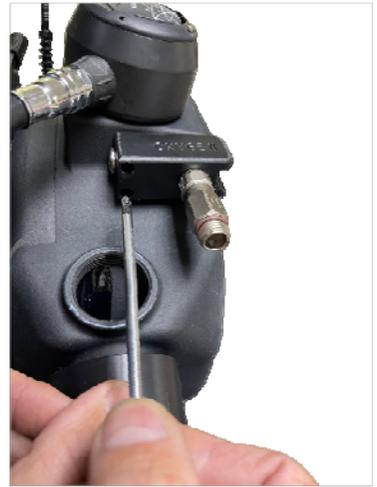

***WARNING: When reassembling the O2 valve, ensure that you do not over-tighten the nut. Remember, when screwing any metal screws into plastic use only two fingers on the wrench. If you over-tighten the nut, it will strip the threads and the valve will leak.**

When attaching the O2 valve to the filter and the hoses, it is very important that you use a second wrench to hold the nut next to the O2 valve body in place. Do not allow this nut to spin as it will over-tighten and strip the plastic. This will cause the O2 valve to leak. The O2 valve body is not a substitute for a wrench.



All low pressure hoses on the DT Go should be inspected periodically to ensure that they are not damaged and in good working order. This includes the oxygen hose and diluent hose.

***WARNING: ALL SERVICE WORK MUST BE DONE BY A QUALIFIED TECHNICIAN ANNUALLY. FAILURE TO DO THIS, MAY CAUSE INJURY OR DEATH!**



Oxygen First Stage Regulator & Flow Rates

The oxygen first stage regulator is located on the bottom of the rebreather and is secured to the on-board cylinder.

The DT Go oxygen first stage is shipped with a delrin block in place. This is different from a standard scuba first stage as the oxygen delivery system on the rebreather must be at a constant pressure, and not variable. The block will prevent the pressure from increasing with depth and increasing the oxygen flow rate.

It is important that both the delrin block and the Over Pressure Valve (OPV) be properly installed on the oxygen first stage. If the delrin block is not installed the oxygen delivery system on the DT Go will not work properly!

The oxygen first stage must only be serviced by a qualified technician annually, that is trained in servicing oxygen clean components.



***WARNING: THE DELRIN PLUG MUST BE PROPERLY INSERTED INTO THE OXYGEN FIRST STAGE FOR THE SYSTEM TO WORK PROPERLY.**

***WARNING: DO NOT EVER USE AN OXYGEN FIRST STAGE WITHOUT AN OVER PRESSURE VALVE! TO DO SO MAY CAUSE SERIOUS INJURY OR DEATH!**

THE OXYGEN FIRST STAGE MUST BE SERVICED BY A QUALIFIED TECHNICIAN ANNUALLY. FAILURE TO DO THIS, MAY CAUSE INJURY OR DEATH!

***WARNING: LIKE ALL PRESSURIZED SYSTEMS, WHEN OPENING THE VALVE'S ON YOUR CYLINDERS, BE CERTAIN TO DO IT SLOWLY!! ALL GAUGES SHOULD BE FACING AWAY FROM YOU. WHEN WORKING WITH PURE OXYGEN, THIS IS EVEN MORE IMPORTANT. FAILURE TO DO THIS, MAY CAUSE INJURY OR DEATH!**

IGNORING ANY OF THE ABOVE WARNINGS, COULD CAUSE SERIOUS INJURY OR DEATH.

Adjusting the oxygen flow rate:

The oxygen injection rate can be adjusted to suit each individual diver. The required flow rate depends on the physical size of the diver and the degree of exertion used during the dive. If the flow rate is too high the PPO₂ will climb to dangerous levels and the breathing loop will have to be purged to reduce the oxygen partial pressure to a safe level. If the flow rate is set too low oxygen will have to be manually added more often during the dive. If you need your flow rate adjusted, seek out a qualified technician or instructor.

***WARNING: TOO LOW IS BETTER AS IT IS QUICKER TO ADD OXYGEN TO THE LOOP, THEN TO FLUSH IT!!**

NOTE: IT IS VERY IMPORTANT THAT TWO WRENCH'S ARE USED WHEN REMOVING HOSES OR FITTINGS FROM THE MANUAL ADD VALVE!!! ONE MUST BE USED TO ENSURE THAT THE FITTING ON THE VALVE DOES NOT SPIN!! SEE THE PHOTOS AT THE TOP OF THE PREVIOUS PAGE WHICH SHOW HOW TO DO THIS PROPERLY.

Flow rate:

What should your flow rate be set at? 0.75 LPM is a good starting point, this is where the DT Go will be factory set. The PPO₂ should remain constant when you are hanging motionless in the water. Try this in a pool for 5 minutes to determine if you need to increase or decrease the flow rate. You should have to add O₂ at regular intervals during the dive due to workload.

WARNING!

The oxygen injector is a convenience. It is not a controller in any way. The only device regulating the oxygen partial pressure is your brain. The automatic oxygen add does not reduce the need to monitor the computer display. It only reduces the number of times you have to press the oxygen add button. The displays should be checked constantly during the dive. The oxygen regulator can fail and stop delivering O₂ or it can fail and increase the flow drastically. The orifice can become plugged and stop delivering oxygen. The add valve O-rings can fail and increase the amount of O₂ being added to the breathing loop. Any of these things can kill you but any of these problems can be overcome if you are aware of the conditions in the breathing loop.

The manual oxygen addition valve is a key component of the DT Go diving system; care should be taken to ensure that it is not damaged, serviced as required and is functioning properly.

**DIVER SHOULD BE CHECKING THEIR PPO₂ DISPLAYS EVERY MINUTE.
KNOW YOUR PPO₂ AT ALL TIMES...OR YOU WILL DIE!!**

Oxygen Manual Add Valve Troubleshooting

If the flow rate is lower than it should be in relation to the pressure, one of the following things has happened:

- The filter has become clogged and should be replaced.
- The orifice has become partially plugged and must be replaced.

DO NOT TRY TO CORRECT A LOW FLOW RATE BY INCREASING THE REGULATOR PRESSURE!

If the flow rate is higher than it should be in relation to the pressure one of the following things has happened:

- The orifice has become loose where it screws onto the valve.
- The valve O-ring is worn or damaged.
- The spring is broken or weakened and is not holding the valve closed.

The oxygen first stage will have a delrin block installed to prevent the pressure from increasing with depth and increasing the oxygen flow rate. If the pressure is inconsistent the high pressure seat or diaphragm may be damaged. The regulator should be serviced regularly and maintained in an oxygen clean condition.

***WARNING: It is very important that this valve is in good working order, with proper flow rates and good O-rings. Ensure that you rinse your gear after diving in salt water, and if you flood your rebreather, and you think water has gotten into the valve, service it!! If you pay attention to how often you usually add oxygen to your rebreather during a typical dive, it will be easier for you to notice a problem.**

Mouthpiece/DSV Maintenance

The following are the steps to service your mouthpiece.

Using an 1/8 inch Allen wrench, reach through the breathing port and remove the screw that holds the lever in place.



Once the lever has been removed, push the inner barrel out. It can be pushed out at either end.




Inspect the inner barrel, and after cleaning it the O-rings can now be replaced. 1 x #121 50 durometer, and 2 x # 127 70 durometer. Next, clean and lubricate the inside of DSV body. Finally, lubricate the outside of the barrel.

The barrel is now ready to be inserted into the DSV body. When inserting the barrel, be certain to align the notch in the barrel with the side of the body that has the small hole.



Inspect the lever, and be certain that the #008 O-ring is in place. Reinstall the lever, being certain to not over tighten.

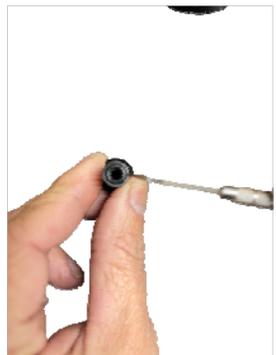

Inspect the mushroom valves, make certain that they are laying flat and will seal properly.

When installing the mushroom valves, the left hand side must allow the gas to flow inwards, from the breathing loop. This is the gas you will be inhaling, and is the scrubbed gas.



The right hand side must allow the gas to flow outwards. This is the gas that you have exhaled, and will be going into the unit to be scrubbed.



WARNING: IF YOU CHOOSE TO CHANGE TO A BOV, IT MUST BE SELECTED FROM A REPUTABLE COMPANY WHICH HAS AN INTEGRATED 2ND STAGE FOR BAIL OUT. AS WELL, THE APPROPRIATE AMOUNT OF BALLAST FOR THE LOOP HOSES MUST BE SECURED. DIVERS WHO CHOOSE TO DO THIS, MUST ENSURE THAT THEY ARE PROPERLY TRAINED TO USE THE BOV.

Mouthpiece Test

Once the mouthpiece has been assembled, it is important to ensure that it is working properly. The following steps will show you how to stereo check your mouthpiece.

1. With the DSV open, cover the right (exhale) side, and blow (gently!!) into the mouthpiece. The mushroom valve should seal and no gas should exit out of the left side.

Problems:

- Mushroom valve on the left could leak. Remove the carrier and inspect it again.

2. With the DSV open, cover the left (inhale) side, and suck (gently!!) into the mouthpiece. No gas should come in.

Problems:

- Mushroom valve on the right could leak. Remove the carrier and inspect it again.

3. Other leaks. Cover both the inhale and exhale sides of the mouthpiece, while gently blowing into the mouthpiece. Also do this test while gently sucking from the mouthpiece. These tests will determine if the rubber mouthpiece has a leak.

4. Attach the loop hoses to the mouthpiece, and with the mouthpiece open, put the open hose ends by your ears. The rubber mouth-bite should be in your mouth. While breathing in and out, you should notice that your exhalation should blow by your right ear, and your inhalation should blow by your left ear. This is called a Stereo Check.

NOTE: CLEAN AND INSPECT THE MOUTHPIECE AS REQUIRED. SERVICING SHOULD BE DONE BY A QUALIFIED TECHNICIAN.

IT SHOULD BE NOTED THAT A LEAK ON THE MOUTHPIECE, INCLUDING THE RUBBER MOUTH BIT, WILL NOT BE DETECTED ON THE POSITIVE AND NEGATIVE TESTS!! THIS IS WHY IT IS VERY IMPORTANT TO KEEP YOUR MOUTHPIECE PROPERLY SERVICED AND CLEANED. ALSO, ALWAYS CARRY A SPARE RUBBER MOUTH-BITE. MOST MOUTHPIECE LEAKS ARE FROM THIS!!

Mouthpiece Servicing & Troubleshooting

***Warning: Your DT Go mouthpiece is a key component of the DT diving system and should be serviced yearly or more often if required. When to service depends on how often you dive, the environment you dive in and also how well it is cleaned after every dive. It is important that it is kept clean and the knob should always turn smoothly. Keeping your DSV clean is important as grit inside the moving parts can score the plastic. Your local DT dealer can assist you with servicing the DSV if you prefer not to do it. Care should be taken to ensure that it is in good working order and not damaged.**

Also, be aware that if you wash your DSV with a powerful hose, the valve disks may be blown off!! After cleaning, be certain to inspect your gear and follow all the pre-dive check's!!!

IF THE MUSHROOM VALVES ARE DISTORTED OR DAMAGED THEY MUST BE REPLACED!!! To remove the old mushroom valve, pull the valve out. To install a new mushroom valve, be certain that you are inserting it onto the flat side of the carrier. Slide the centre stem through the hole. Gently pull it through until it clicks into place.

WATER INTRUSION

First determine if the water is sea water (from diving) or fresh water (if you are not fresh water diving, this could be condensation).

If it is sea water, service your DSV and ensure that the O-rings are all in good shape. Also clean and lubricate at this time.

Check your rubber mouth bite for damage and for a proper fit onto the mouthpiece. They generally come in a variety of attachment sizes. Ensure that the one you choose fits properly. There are some specialized rubber mouth bites which while a pleasure to dive, just do not fit properly on our mouthpiece. Seacure is one of them and after time it will always leak.

Also check for a tear underneath the zip tie which holds the rubber mouth bit in place. Damage here will also cause water to leak into the system.

Many cases of water into the loop come from torn or damaged rubber mouth pieces.

Loose lips.

Your loop hoses should be inspected around the hard connections for a pinch or tear.



Loop Hoses & Hose Stubs

The DT Go is shipped with a quick connect system for the scrubber side of the loop hoses. You will see that the towers on the scrubber head have a lip in which the quick disconnect hose stubs are secured. The unit is shipped standard with 2 hose stubs which will be fitted to your loop hoses with hose clamps, prior to shipping.

***NOTE: THE TOWERS ARE THREADED INTO THE SCRUBBER HEAD AND SEAL WITH AN O-RING. WHILE THE TOWERS ARE DESIGNED TO BE DIFFICULT TO TURN, IT IS STILL IMPORTANT THAT THEY ARE NOT ACCIDENTLY UNSCREWED WHILE REMOVING OR INSTALLING THE BREATHING HOSE. A LOOSE TOWER WILL LEAK!!! CHECK THE TOWERS PRIOR TO DIVING TO ENSURE THEY ARE TIGHT.**

The procedure to install the hose stubs to the towers are as follows:

- Ensure that the sealing areas on the towers are clean.
- Ensure that the O-ring areas on the hose stubs are clean and then apply lubricant.
- Push the hose stub on to the tower, lining up the lip on the tower with the space on the hose stub.
- Turn the ring to secure.
- Inspect the area to ensure that all the O-rings are properly seated and not pinched.
- To remove the hose stub, push in on the stub, and then turn the ring. This is a similar method to opening and closing a child proof medication bottle.



***SERVICE: THE O-RINGS ON THE HOSE STUBS AND THE CORRESPONDING SURFACES ON THE DSV ADAPTERS AND HOSE ATTACHMENTS SHOULD BE LUBRICATED ON A REGULAR BASIS. PRIOR TO DIVING, ENSURE THAT HOSES HAVE BEEN PROPERLY ATTACHED TO THE TOWERS AND TO THE DSV!!! FAILURE TO DO SO COULD CAUSE INJURY OR DEATH!!!**

Diluent Cylinder & Quick Connect System

The diluent cylinder on the DT Go is back-mounted similar to a standard diving system, and doubles as the diver's bailout system. In this configuration the diluent cylinder is referred to as off board diluent gas as the cylinder is not secured to the main rebreather. The advantages of this are that diver's may customize the system to suit their diving needs. It also keeps the main rebreather small, light, flexible, and easy to travel with.

DT recommends that a minimum of 40 cuft should be used as the diluent/bailout cylinder when diving recreationally. Diver's must be certain that the cylinder they choose has the proper amount of gas for diluent, wing & drysuit inflation, and also for bailout. Those doing any sort of technical and/or decompression diving must carry a larger cylinder(s) and ensure that it is appropriate for the dive that they are planning.

The DT Go includes a low pressure quick connect. This accessory is used to plumb the diluent/bailout gas into the rebreather via a low pressure inflator hose.

The low pressure inflator hose should be secured to the diver's first stage on the diluent/bailout cylinder.

***WARNING: AS WITH ANY NEW DIVING EQUIPMENT, USING THIS ACCESSORY WILL REQUIRE THE DIVER TO LEARN NEW SKILLS AND CREATE NEW MUSCLE MEMORY.**



INSERT UNDERWATER PHOTO HERE.

Filling the Scrubber Canister

The DT Go has an axial scrubber design, which is resistant to channelling. It holds approximately 3.5 lb/1.59 kg of absorbent. The actual weight will depend on the brand that is used. (Divers must use 8-12 granule size)

***WARNING: The use of larger granules can cause channeling. This can cause serious injury or death!**

The Go has a unique design with a large face, which has a lot of surface area. It also has a short bed length. This spreads out the exhaled gas, which lowers the breathing resistance. (breathing resistance is also known as Work of Breathing, or WOB).

The procedure to fill the scrubber canister is as follows:

- Remove the top screen.
- Fill the canister with absorbent, about half way up.
- Tap all the sides of the canister to help settle the absorbent.
- Add more absorbent, as needed, until the level is 1/8 inch below the absorbent fill line.
- Put the top screen in place, over the absorbent.
- The top screen will need to be wiggled back and forth to settle the absorbent.
- While putting light pressure on the top screen, tap the edges again. The fill line should be slightly visible above the screen.



- Using a lint free cloth or paper towel, clean the O-ring surface area of any debris or grit.
- Using clean fingers, apply a light amount of lubricant to the O-ring surface area.



- Place the lid in position, being certain to align the clamps.
- Gently press the lid straight down to push it into position. It should easily be pushed down, moving smoothly and evenly.
- Visually inspect the scrubber canister, and make certain that there are no gaps between the canister and the lid.



***WARNING: IF THERE IS A GAP BETWEEN THE SCRUBBER CANISTER AND THE LID, IT IS LIKELY DUE TO A PINCHED O-RING!! IF THIS HAPPENS WATER WILL LEAK INTO THE SCRUBBER CANISTER & UNIT, WHICH WILL RESULT IN A CATASTROPHIC FAILURE!!!!**

Duration:

Cold water, below 12.7°C/55 °F : 1.5 hours

Moderate water, 12.7°C/55 °F to 21.1°C/70°F , 2 hours

Warm water, above 21.1°C/70°F: 2.5 hours

***WARNING: Diver's have been known to travel great distances with their rebreather's assembled and the scrubber canister packed. A word of warning; the greater the distance traveled the more likely the absorbent can settle with the large and small granules separating. This could cause channeling, which in turn could cause a problem with Carbon dioxide, which could cause serious injury or death. How to avoid this? Travel shorter distances only. Also it is far less likely to happen if you travel with the rebreather in a flat position rather than having it vertical, as laying it flat will decrease the chances of the absorbent settling to one side. If you have concerns about this, it is better to pour out the absorbent once you reach your destination, and repack it. Remember, this can happen on any rebreather!**

***NOTE: The scrubber assembly, is a key part of the rebreather and care should be taken to ensure that it is not damaged and is working properly.**

***WARNING: IF CANISTER O-RING IS PINCHED AND THERE IS A LEAK, YOU WILL HAVE A SERIOUS FLOOD!!! THIS COULD CAUSE SERIOUS INJURY OR DEATH!!**

Counterlung Installation

The counterlung system on the DT Go consists of 2 equal sized lungs, which are approximately 2.3 litres each.

- Visually inspect the O-rings on each counterlung. Ensure that they are in place, and in good condition. They should be wiped clean with a lint free cloth or paper towel, ensuring no debris or grit is present.
- The right side counterlung has an over pressure valve (OPV) installed. Inspect the OPV to ensure that it is clean, with no debris or grit present, and then ensure it is tightened all the way in.



- Ensure that the inside of the counterlung adapter is clean, and free of any debris or grit. To the inside of the counterlung adapter, apply a light amount of lubricant.




- Press the counterlung release, and insert the counterlung. Use smooth and even pressure.




- Once the lung is in place and properly secured, ensure that it is properly angled. It should be similar to the photo.



- Once the lung is properly installed, secured and properly angled, the counterlung retaining quick-link should be installed.

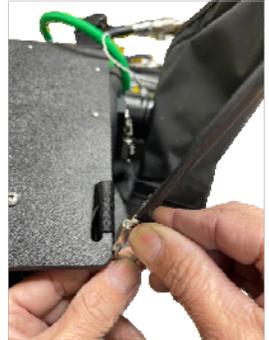

- The quick-link should be screwed down tightly.

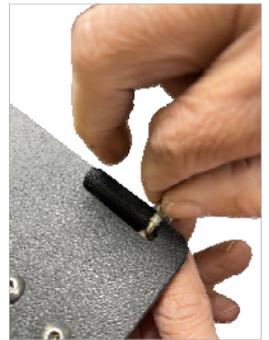

- Follow the same installation procedures to install the left side counterlung.

Loop Hose & DSV Assembly

Lubricate the inside of the hose end.



Inspect the O-rings. Then, gently slide the hose attachment onto the DSV, being careful not to pinch the O-rings, or cause them to extrude.



To insert the retaining clip, squeeze it gently, and push it into the groove. Repeat with the other side.



Our DSV has a larger bore and has an excellent work of breathing. In order to get that good work of breathing, the valves are more flexible. This means that with this, we need to ensure that we have good testing habits. Those divers who learned the testing procedures years ago, have to understand that the equipment has now changed, and that our habits must also change.

Also ensure that the area where the Mushroom valve seal's is clean. build up in this area will cause the diaphragm to leak.

Positive/Negative Testing

Once the DT Go has been completely assembled you are ready to do the positive and negative pressure tests. While these tests will give you the best indication of any leaks in the system, it is still a good idea to do a quick bubble check when you enter the water. That's where buddies come in handy.

***WARNING: IT IS VERY IMPORTANT THAT THE POSITIVE/NEGATIVE PRESSURE TESTS ARE COMPLETED AND THAT THEY ARE DONE PROPERLY. ANY LEAKS THAT ARE PRESENT ARE MOST LIKELY TO BE CAUGHT WHILE DOING THESE TESTS!! WHEN DOING YOUR TESTS, YOU SHOULD BE VERY CERTAIN THAT THEY PASS. IF YOU HAVE ANY DOUBT AND ARE UNSURE THAT THE TEST PASSED, YOU PROBABLY HAVE A SMALL LEAK. FIND IT!! THE UNITS HOLD VERY GOOD POSITIVE AND NEGATIVE TESTS.**

To do the negative test, first ensure that the male end of the off board accessory is plugged. All gases should be off, the unit fully assembled, exhaust valve closed. Then put the DSV into your mouth, turn the knob and inhale the gas from the loop into your lungs and exhale it out of your nose until it is impossible to inhale any further. When the loop is empty, there should be no leakage into the rebreather and you shouldn't feel any extra gas sneaking into your mouth. If you don't feel any extra gas, close the loop while inhaling. The breathing hoses should be tighter as there is a vacuum in the loop. This will cause the DSV to sit higher than usual and the ridges on the hoses to be close together. If you watch the hoses while you are drawing the gas out of the loop, you will see how they constrict. Also, look at the counterlung's. They should be completely flat. Once you close the mouthpiece, watch the hoses and lungs closely. Don't look away. You need to notice if anything changes, such as a slight droop in the hoses and/or the mouthpiece dropping or the lungs shift slightly showing that gas might be going back into them. Leave the loop closed for a few moments, 60 seconds is adequate, to see if the vacuum holds and then open the loop to let air back in. (Longer is not necessary and will damage the diaphragm.)

The next most important part of doing your negative test (watching the lungs and hoses is the first) is when you release the pressure and open the mouthpiece. You should hear a “whoosh” as pressure is released. If you don’t hear this sound, you have a leak! Or if the “whoosh” isn’t as strong as it usually is, you have a leak. After diving the unit for a while, you will learn what sound to expect when releasing the pressure. When you hear that sound, you will feel confident that you did a good test. If you have any uncertain feeling, then you may have a small leak.

***WARNING - It is important to not leave the vacuum in the loop for more than a few moments as this will cause damage to the diaphragm. If this happens, the ADV will not work properly. It will either stop working altogether or will continuously feed the diver diluent. It will certainly allow water to leak into the ADV.**

***NOTE: When doing your test, it is VERY important to not suck so hard that you are damaging the diaphragms. When you do the negative test, suck until you get a good seal, and then immediately close off the DSV. if you suck so hard that you feel the pressure building in the back of your throat/neck area, your ears pop, or you feel your face turning red for exertion, this is way too hard. There is no need for this and it will damage the valves and diaphragms. Suck just until you feel that pressure, then close the valve.**

To do the positive test, put the DSV into your mouth, turn the knob and exhale into the loop until you hear the exhaust valve release and then quickly close the DSV without letting any air escape the loop. The counterlung's should be expanded to their maximum size. Listen carefully for any air leaks and ensure that the counterlung's remain firm for several minutes. The oxygen tank valve and mouthpiece should be closed during these tests. After the test is complete and you open the DSV again you will hear the sound of the pressure being released. This is important!



Dive Computer & Calibration

The DT Go uses the Shearwater display and monitoring system, which utilizes the 4 pin connection system. Options are:

- Shearwater Petrel wrist computer with the 4 pin connection system.
- Shearwater NERD with the 4 pin connection system.
- 4 pin connection system only.

Adjusting the oxygen flow rate:

The oxygen injection rate can be adjusted to suit each individual diver. The required flow rate depends on the physical size of the diver and the degree of exertion used during the dive. If the flow rate is too high the PP02 will climb to dangerous levels and the breathing loop will have to be purged to reduce the oxygen partial pressure to a safe level. If the flow rate is set too low oxygen will have to be manually added more often during the dive. If you need your flow rate adjusted, seek out a qualified technician or instructor.

All computer instructions may be found in the Shearwater manuals.

***WARNING: IT IS CRITICAL THAT ALL DT GO DIVERS READ AND FULLY UNDERSTAND THE SHEARWATER MANUALS AND ALSO FULLY UNDERSTAND THE CALIBRATION INSTRUCTIONS. FAILURE TO DO SO COULD CAUSE SERIOUS INJURY OR DEATH!!!**

***WARNING: Never risk your life on only one source of information. Use a second computer or tables. If you choose to make riskier dives, obtain the proper training and work up to them slowly to gain experience.**


***WARNING: All display system's will fail. It is not whether it will fail but when it will fail. Do not depend on it. Always have a plan on how to handle failures. Automatic systems are no substitute for knowledge and training. No technology will keep you alive. Knowledge, skill, and practiced procedures are your best defense. (Except for not doing the dive, of course.)**

***WARNING: DIVERS THAT CHOOSE TO PURCHASE THE DT GO, WITHOUT THE COMPUTER OR NERD, MUST ENSURE THAT THEY ARE USING AN APPROVED SYSTEM. FAILURE TO DO SO MAY CAUSE SERIOUS INJURY OR DEATH.**

Calibration:

Attach an oxygen cylinder to the first stage. Most divers will use a separate larger cylinder, so the cylinder that is actually used on the dive is not depleted.

Once attached, open the cylinder valve.

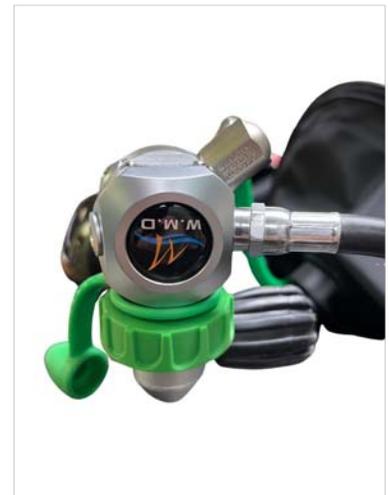

Open the DSV.



Turn on the computer, and set to calibrate.



Press the oxygen MAV button and watch the PPO2 rise.

When the millivolts level out, press calibrate. (right button)

The Millivolt reading will be between 9 and 13 millivolts, in air. As long as they are in that range, they are safe to use. In 100% oxygen, at sea level the sensors should be between 40 and 60 millivolts.



It will give you report with altitude. Confirm by pushing the right button.



This completes the calibration process, and shows the PPO2 value on the screen. If you are at sea level this will be 0.98. The higher the elevation, the lower the equivalent will be.



INSERT UNDERWATER PHOTO HERE.

Pre-dive Checklist's

The first part of our check list, are items that must be addressed and/or confirmed prior to suiting up for the dive. Those that are using this tool, usually keep several blank copies in a small binder with their dive gear.

The second part of the check list are items that are usually checked shortly before a dive. This list can also be printed out, but other options are to copy it onto a dive slate or wet-notes in a permanent ink marker.

A point worth noting is that all pilots have a check list which they go through every time they fly. Diving a rebreather should be no different. While rebreather diving doesn't necessarily take more preparation or clean up time than open circuit diving, there are very specific things that need to be checked and confirmed prior to getting into the water.

Using this check list will only add a few seconds more time to your preparation, but could make all the difference in having a pleasurable time in the underwater environment. It certainly assists in creating competent, happy divers.

DIVERS SHOULD FOLLOW THE PRE-DIVE CHECKLISTS BEFORE EVERY DIVE AND KEEP A COPY OF THE CHECKLIST WITH THE DT GO AT ALL TIMES.

Dive Talk GO Build Checklist

- Check and lubricate scrubber O-ring
- Fill scrubber to 1/8" below fill line and place screen
- Do not overfill the scrubber
- Secure lid in place
- Attach counterlungs
- Stereo check DSV
- Attach breathing hoses
- Attach oxygen cylinder
- Attach Shearwater Petrel or NERD
- Check PPO2 and millivolts in air (sensors should be 8.5 – 13 millivolts in air)
- Check battery life
- Verify gases for CCR and bailout - gas mixtures & cylinder pressure
- Reset stack timer
- Turn on oxygen, check pressure, and verify function of oxygen manual add valve
- Turn off oxygen and watch pressure fall to verify leaky valve is functioning
- Positive pressure check
- Negative pressure check
- Calibrate oxygen sensors using 100% oxygen (on 100% oxygen, each sensor should read 4.76 times the millivolts they read in air)
- Attach to regulator via low pressure hose, and verify ADV and MAV function of the regulator

Post Dive Checklist - DT GO Disassembly

After diving the DT Go, your diving system will need to be disassembled and cleaned. Follow the disassembly procedures at the front of the manual; follow with the cleaning instructions below.

- Rinse the rebreather, wing & harness fully with fresh water. Be certain to rinse the first stages, valves and any regulators very well.
- The loop components should be rinsed and sanitized after diving. In order to disinfect the components, a product such as Virkon must be used. Virkon is a product that comes in powder form which must be mixed with water. Follow the package directions for use.
- After sanitizing, rinse all components in fresh water. Set out to dry. Counterlung's can easily be dried by turning them partially, inside out.

Once your components are dry, the unit may be stored for future use. Keep in mind that it is best to not store the unit assembled. The O-rings will get a memory and not seal as well.



Troubleshooting - Exhaust Valve, ADV & Work of Breathing

In this section, you will find information about the exhaust valve, ADV and work of breathing. We have helpful hints and trouble shooting. The exhaust valve and the ADV work in harmony. If you are having difficulties with either one, it makes sense to check both.

BUBBLING OVER PRESSURE VALVE

There are several things that can cause this problem. Over the next few pages, situations are listed and described.


1. ***There is debris in the valve.*** See below for instructions on how to take the valve part, should you need to.

It should be noted that if the lungs on the unit are full, and you then open the mouthpiece and start breathing while on the surface, you will find that the air is difficult to exhaust through the exhaust valve. If this happens, it will feel like you can't properly inhale or exhale fully. This generally happens after a diver does his pre-dive testing and pre-breathe and the unit's lungs are inflated. To solve this problem, simply exhale gas out of the loop through your nose. Under-water, the exhaust valve will dump the gas for you.

OVER PRESSURE VALVE MAINTENANCE



1. Unscrew from the counterlung.

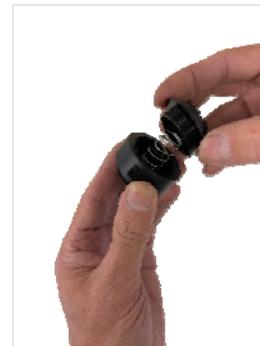

2. Unscrew the top.



3. Remove the spring and piston




4. Flush water through from the backside.

3. **ADV problem.** If your counterlung volume is correct and the exhaust valve is in good working order, and you still have a leaking exhaust with the feeling of too much gas in the loop, you could have a problem with your ADV adding too much gas into the system. If this is happening you will also notice that your PPO2 is reading lower than usual and that your buoyancy is off. This could be caused by a stretched, damaged or torn ADV diaphragm, or a problem with the other components of the ADV. Inspect the diaphragm for damage or fault. If you have an adjustable ADV, have it serviced by a qualified technician.

To determine if this is the problem, shut off the diluent gas. First you will notice your PPO2 stabilize and stop dropping. Also, the lungs will stop filling up all the way and the exhaust valve should stop purging.

The diaphragm is simple to check. Open the cover and pull the assembly out. It should be fairly flat, and not damaged. You may need to look quite closely for small tears or holes. Sometimes holding it up to the light and gently pulling the rubber will help. When you reinstall the cover, tighten the bolts to inch pounds.

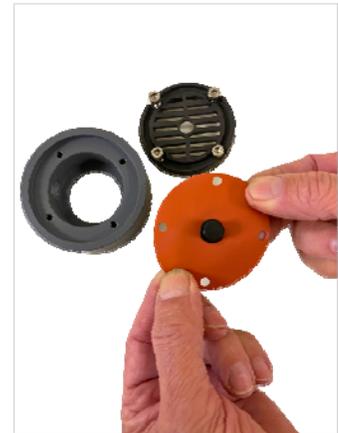

4. **Check the IP on the diluent first stage.** It should be between 8 (117.6 psi) and 10 bar (147 psi).
5. **First stage needs to be serviced.** If the first stage is not functioning properly, it could have a leak, which could cause excess diluent gas to flow into the rebreather's loop.

***NOTE: A damaged ADV assembly will either deliver too much diluent gas, or none at all.**

***NOTE: It is important that the proper installation procedures are followed for the ADV assembly and diaphragm. Only qualified technician's should service the regulator. Those with no experience should take it to their local DT Go dealer or send it to the DT Go head office for servicing. The exhaust valve is a key component of the DT Go diving system; care should be taken that it is not damaged and properly maintained.**

ADV IS DIFFICULT TO TRIGGER

The position of the diver will effect the ADV. If the diver is horizontal or face down, the ADV will trigger easily. If the diver is vertical, then it will be a bit harder. Also, rolling to your right side, while horizontal, will assist in triggering the ADV.

Lastly, check the IP on the diluent first stage. Ensure that it is in the correct range. Remember, the ADV is not meant to be easy to trigger. It was designed this way so that the diver would know when they were triggering it. If it was too easy, then diluent gas could be fed into the breathing loop without the diver being aware of what was happening.

WORK OF BREATHING

There are several things that can cause a high work of breathing.

1. ***Too much gas in the loop.*** This can happen if the loop has gas in it, the mouthpiece is closed and then the diver puts the mouthpiece in his mouth and blows more gas into the loop. The exhaust valve will probably not release any gas if the diver is on the surface. It will feel like you can not get a full breath and the breathing will be difficult. Dump part of the loop (exhale out of your nose). If this is the cause, you will notice the difference immediately. Also, if this happens, it won't be possible to trigger the ADV. This can also happen if the ADV is faulty and it is leaking diluent gas into the loop.
2. ***Twisted counterlung's.*** If the counterlung's are twisted, or bunched up, they will not be able to expand properly and breathing will be restricted.
3. ***Counterlung's not attached to the frame properly.*** If the counterlung's are not properly routed, it is likely that they could be restricted in some manner. This will cause the breathing to be restricted.



Warranty

The Dive Talk Gear, LLC. rebreather and DSV are warranted for the period of 1 year. All warranty and service work should be returned to our warehouse.

- The warranty applies to the original owner only.
- Mistreatment or neglect of the products will void the warranty.
- Parts not covered by the warranty are batteries and sensors.
- Completed liability waivers must be on file for the rebreather warranty to be valid.
- Modifications to the DT Go will void the warranty. Only approved modifications are allowed.
- We are unable to determine if the parts are covered by the warranty until they have been inspected.

PROCEDURES FOR WARRANTY & SERVICE WORK

Prior to shipping, please email info@divetalkgo.com to inform us of your shipment. You will need to print out the warranty/service form, fill it in and ship it with your item. This form can be obtained from the DT website at www.divetalkgo.com

Your product should be returned to us with the warranty/service form, in the box.

Carefully box up the items being returned. Dive Talk Gear, LLC. is not responsible for any damage incurred during shipping. Ensure that the items are properly padded and shipped in a strong box, and also that it is well sealed. (Don't forget to insert the above mentioned paperwork!) Please write in large clear letters, WARRANTY RETURN, MADE IN USA on the outside of the parcel and on any paperwork. This is important as otherwise USA Customs will charge us a brokerage fee and duties, which we pass on to you.

The parcel may be shipped via the post office or a courier. All shipments must be prepaid and insured. Any fees that Dive Talk Gear LLC. incurs must be paid for by the shipper. This includes duties and brokerage fees for the item re-entering the USA. Note that if you ship via a courier such as UPS or Federal Express, there will be a brokerage fee, even if there are no duties. While there may be no charges for the warranty work, this brokerage fee must be paid for by the shipper.

Dive Talk Go - Information Sheet for New Divers

What is Dive Talk Gear, LLC. doing to ensure that divers understand how to safely use their products?

It is the duty of all rebreather manufacturers to ensure that when a diving system is sold, our clients are able to confidently choose a Training Agency and Instructor that will fulfill the training requirement.

In our goal to help divers become the best rebreather diver's possible, Dive Talk Gear, LLC. has a Training Quality Assurance program (TQA), which outlines our standards and expectations.

As a Dive Talk Go rebreather owner, there are some things we would like you to know:

1. Dive Talk Gear, LLC has 2 private Facebook groups, Dive Talk Go Divers, and Dive Talk Go Instructors. We strongly recommend that all DT Go owner's join the DT Go divers' group, and all instructors join the DT Go instructor group. While these lists may not be terribly active, it is where we release important information such as manual updates, issues, recalls, etc.

Dive Talk Go rebreather owners should search Facebook for, Dive Talk Go – Official Page. Dive Talk Go rebreather instructors should search for, Dive Talk Go Rebreather Instructors – Official Page. If anyone is having difficulty finding these pages, please email us at, info@divetalkgo.com for help.

Upon asking to join, you will be asked a few questions. Upon receipt of your request and answers, your membership will be granted.

2. You will find a copy of the Dive Talk Go minimum training standards in the back of your manual. We have published it here as we feel it is important for all DT Go divers to understand what the minimum training requirements are for each level of training. DT Go approved training agencies are able to add to these standards, but not take away from them.
3. Also, in the back of your manual are copies of the Dive Talk Go rebreather course evaluation form. As you can see the form lists all the required skills, and your score. At the completion of the program, all students and instructors are required to sign off/date this form. Your instructor will email the final copy of the form to Dive Talk.

Again, we have published these forms so that all DT Go owners know what to expect in their training program. As a DT Go diver, you have made an investment in a specialized piece of diving equipment, and in a specific training program. As such, you deserve to receive the equipment as promised, and all the training that you have paid for. If at any time you feel that this hasn't happened, please contact us directly at, info@divetalkgo.com.

4. Anyone that purchases a DT Go rebreather, must have the appropriate training.
5. The Dive Talk Go Training Quality Assurance (TQA) information is listed on our website, www.divetalkgo.com. Here you will find copies of the minimum training standards, course evaluation forms, Instructor Registration forms, and other information.

6. As a number of our sales go through our dealers, we don't have contact information for all our divers. We ask that all Dive Talk Go divers ensure that they are registered with us, so we are able to reach you should the need arise. As mentioned, we do publish information on our private Facebook groups, and in other places, but having your name and email address (at a minimum) on file with us would help insure that we can reach you in the event that we have important information. Ideally please email us your: full name, address, phone number, email address, the name of the unit you are diving, and your serial number. This information can be sent directly to, info@divetalkgo.com.

Dive Talk Gear, LLC has a duty to their clients to ensure that Dive Talk Go divers understand how to safely use their products. We take this very seriously. If anyone ever has a concern, comment, observation, we would love to hear from you. Our goal is to be the best that we can, and feedback from our clients will help us achieve that. Any feedback may be emailed directly to us at, info@divetalkgo.com.

RESA recommends: Dive Rebreathers safely by following this 10 point plan

1. Be wary of “internet advice”. Check the manufacturers and training agencies for best practise/configuration information and if you can’t find the information you need, contact them.
2. Take time to learn your rebreather and practise using all the controls regularly.
3. Use a checklist before every dive, for assembly and pre-dive checks, ensuring that when you get in the water you haven’t forgotten something stupid:
 - a. Ensuring everything is okay BEFORE you get in the water increases the chances exponentially of it being a successful, trouble free dive.
 - b. We’re all human, we all forget things, but you’re entering an environment where even trivial issues on the surface can be fatal underwater.
 - c. No matter what your experience level, it is stupid not to use a checklist system, whether it be electronic or paper – use a checklist.
4. Unless the manufacturer of your unit advises differently, change your oxygen sensors every 12 months — O2 sensors/cells are a consumable. Their useful life is much less in a rebreather than in a surface O2 analyser:
 - a. Several diving professionals have lost their lives over the past few years because they didn’t change their cells in a timely fashion.
 - b. Understanding what current limiting is and what to do about it are important skills. Test for it on every dive by adding a little bit of oxygen to see whether the cell rises by 0.1 bar or not, and if not start reducing your setpoint down below 1.0 bar or more or bailout to open circuit.
5. Dive with a buddy. Be a buddy. Most rebreather divers are capable of diving alone but it is always useful to have a friend to help identify that your dry suit hose isn’t connected yet or is on hand to help reach components. A good buddy is a good diver. A good diver is a good buddy.
6. Take your time. Take time to sit and think about the dive, about your equipment. Is everything connected? Is everything working properly?
7. Plan your bailout requirements:
 - a. Ensure you have enough bailout gas for the planned dive.
 - b. Ensure you can reach bailout.
 - c. Test your bail-out pre-dive and early in the dive.
 - d. If your “emergency plan” is your open circuit bailout, make sure you use it. Too many divers die carrying bailout.
8. Use only the CO2 absorbent and grade recommended by the manufacturer, that is the grade tested in their machine and has known performance:
 - a. Some absorbents are totally unsuitable for diving, they just don’t absorb CO2 quickly enough.
 - b. If you do use a different diving grade absorbent to that recommended, you MUST reduce the usage time. If the absorbent has a larger granule size than that in the recommended absorbent, reduce the usage time by at least one third.
 - c. Changing it early is much better than changing it late. Push the scrubber to it’s limits and one day you will be caught out.

9. Don't be afraid to cancel a dive. You are part of the pre –dive analysis. If you don't feel right or have misgivings about the dive, just cancel it, walk away. The dive will be there tomorrow and the next day and the day after that:
 - a. Be a good buddy, respect your buddy's wishes – if s/he wants to cancel then so be it, they're safer on the boat.

10. Do pre-jump tests & re-check with appropriate safety drills when you jump in:
 - a. Check PO2 on HUD and handset and continue to do so regularly during the dive.
 - b. Check both tanks are on.
 - c. Check buddy.
 - d. Leak check prior to dive and always bubble check in the water.



Dive Talk Go – CCR Diver Course Evaluation Form

As per the DT Go minimum required training standards, the course must be completed with the minimum required dives and minutes, along with discussion on required academic topics, and all required skills. The student must achieve a minimum score of 8 out of 10 points in all the following skill areas.

DT Go minimum training standards may differ from approved training agency standards. As DT Go minimum training standards are the minimum required standard, the approved training agencies may add to them. Instructors should check with the appropriate training agency to ensure that all standards have been met.

Student: _____ Instructor: _____
Course start date: _____ Course completion date: _____
Dive Talk Go model & serial number: _____

Skills:

1. Pre-dive checks: Average score: ____
 - ____ Specific unit checklist
 - ____ Verify diluent and oxygen (O2) cylinder contents using gas analyzers
 - ____ Unit built up
 - ____ Scrubber canister filling
 - ____ Breathing loop check including mouthpiece one way valves and positive and negative check
 - ____ Sensor calibration in oxygen, with verification in air
 - ____ 5 minute pre-breathe
 - ____ Bailout bottle/stage cylinder rigging
2. Demonstrate correct pre-dive planning procedures: Average score: ____
 - ____ Limits based on system performance
 - ____ Limits based on oxygen exposures at chosen PO2 levels
 - ____ Limits based on nitrogen absorption at planned depth and PO2 set point
 - ____ Appropriate selection of decompression conservatism/gradient factors for the planned dive
 - ____ Thermal constraints
3. Underwater verification: Average score: ____
 - ____ Stop at 3-6 meters/9-19 feet on descent for leak bubble check
 - ____ Counterlung and Over Pressure Valve adjustment, if necessary
4. Mouthpiece familiarity skills: Average score: ____
 - ____ BOV: switch between open and closed circuit
 - ____ DSV: switch to bailout system
5. Adding diluent gas/ADV familiarity skills: Average score: ____
 - ____ ADV: Adding diluent gas and understand how it works
 - ____ BOV: Use BOV to add diluent gas to the loop – 2 ways
 - ____ Bail out second stage: Use to add diluent gas to the loop
 - ____ Dual button MAV: Adding diluent gas (if unit is shipped with this item)

6. Emergency procedures: demonstrate appropriate response to the following; each dive should have a minimum of 2, "diver emergencies" that the student must react to: Average score: ____
 - ____ Practical bailout skills: including 2 open circuit ascent's from approximately 18 meters/59 feet
 - ____ Gas shut downs and loss of gas
 - ____ Broken hoses
 - ____ Flooded absorbent canister
 - ____ Carbon dioxide (CO2) breakthrough
 - ____ Low oxygen drills
 - ____ High oxygen drills
 - ____ Flooding loop
 - ____ Electronics, sensor, and battery failure
7. Practice transferring to open circuit bailout: Score: ____
8. Rescue skill session as outlined by Training Agency: Score: ____
9. Use of buoyancy control system: Average score: ____
 - ____ Buoyancy and trim control at safety stop
 - ____ Buoyancy and trim control during dive
10. Controlling and monitoring for PPO2 levels: Average score: ____
 - ____ Raising/lowering PPO2
 - ____ Starting PPO2
 - ____ PPO2 monitoring every minute
 - ____ Manual Add Valve verification: static at constant depth, monitor change over several minutes
 - ____ Electronics systems monitoring for PPO2 levels (SETPOINT) and setpoint switching using manual and pre-programmed methods when available (when the unit is equipped with an on board decompression computer that monitors sensors)
11. Electronic systems use: Average score: ____
 - ____ Use and adjustment of Heads Up Display, position, brightness, colour
 - ____ Use and adjustment of PPO2/depth/time display, position, brightness, colour
 - ____ Use and adjustment of decompression computer, set up/gas switching, battery verification, etc
12. Use of lift bag/DSMB and reel (where relevant and applicable): Score: ____
13. Mask removal and replacement: Score: ____
14. Proper execution of the dive within all pre-determined dive limits: Score: ____
15. Demonstration of safety stops at pre-determined depths (on all dives): Score: ____
16. Constant loop volume management: Score: ____
17. Cell validation checks with appropriate use of diluent and oxygen: Average score: ____
 - ____ Oxygen sensor verification at depth
 - ____ Linearity check of sensors at approximately 5 meter/16 feet on pure oxygen
18. Post dive cleaning of unit: Average score: ____
 - ____ Mouthpiece and hoses
 - ____ Clean and disinfect unit

____ Inspect components of unit

19. Diver maintenance of unit: Average score: ____
____ Cell removal and replacement
____ Mouthpiece care
____ Replacing or re-charging of batteries

20. Demonstrate an adequate level of fitness by completing a minimum of a 50 meter/164 feet surface diver tow with both rescuer and the victim wearing a complete CCR diving system and bailout cylinder(s) applicable to their specific program: Score: ____

21. Complete all academic sessions and unit specific assessments as specified in the training material of the training agency and the manufacturer: Completed: ____

22. Complete a minimum of seven (7) training dives, including confined water skill development of at least one (1) hour, and six (6) core open water training dives with a minimum run time of 30 minutes each: Completed: ____

23. Complete a minimum of 420 minutes of total in-water time (including confined water) on the applicable unit: Completed: ____

24. Be able to independently complete a dive plan: Completed: ____

25. Complete the final course exam as set out by the training agency with a required minimum pass rate of 80% with 100% remediation: Completed: ____

Student Signature: _____ Date: _____
Instructor signature: _____ Date: _____

In order to complete the students Dive Talk Go certification, this document must be completed in full, and emailed to: info@divetalkgo.com.

PLEASE PRINT CLEARLY - IF WE CAN'T READ YOUR WRITING, WE CAN NOT PROCESS THIS FORM.
THANK YOU!

CCR DIVER

INTENT

The CCR Diver program provides divers with the knowledge and training necessary to independently plan and conduct unit specific no decompression closed-circuit rebreather (CCR) dives to a maximum depth of 30 meters/98 feet, using a manufacturer approved CCR unit with air as diluent utilizing CCR Diving procedures with a dive buddy diving on a rebreather or diving open circuit.

REQUIRED INSTRUCTOR RATING

An active status unit-specific CCR Instructor or higher may conduct the unit-specific CCR Diver program.

TEACHING RATIOS

- The maximum number of students for CCR training is 3:1
- The maximum number of students for no-decompression CCR training where one (1) student is making a crossover or doing a refresher is 4:1

These ratios should be reduced as required if the situation and/or environmental conditions call for it.

STUDENT PREREQUISITES

- Nitrox certification
- Have logged 20 open water dives
- Minimum age: 18

DURATION

- Recommended hours for course completion: 40
- Minimum number of days: 4
- Minimum number of hours for Academics and Dry practical: 8

MATERIALS AND EQUIPMENT

The minimum required student and instructor equipment for this program includes:

A complete DT Go CCR Unit that:

- Is compliant to local laws, is approved by the training agency and is properly functioning
- Has no non-manufacturer approved modifications
- Depth gauge & bottom timer, or dive computer
- A single off-board bailout gas suitable for a safe return to the surface from the planned maximum depth including all safety and decompression stops in the event of an emergency
- For Open water and lake environments with the exception of cave/overhead environments a Delayed Surface Marker Buoy (DSMB) and a spool / reel appropriate for the planned dive depth.
- cutting device
- Access to an appropriate gas analyzer

The minimum required student and instructor materials for this program includes:

- DT Go Rebreather unit specific user manual
- Agency student training manual or online training course
- Agency instructor manual (electronic instructor manuals meet this requirement)
- Course liability release and assumption of risk (in accordance with local laws)
- Training agency approved medical document
- Unit specific checklist (units equipped with a built in electronic checklist, meet this requirement)

- Manufacturer's sign off sheet/course completion document

All skills must be demonstrated by the instructor on the specific unit being trained

REQUIREMENTS FOR COMPLETION

Academics

Students shall have sufficient understanding and knowledge in the following subject areas listed. They should be capable of planning dives in the typical local conditions and environment and be able to plan for typical emergency situations.

1. Practical mechanics of a CCR
 - Assembly and disassembly specific to DT Go rebreather being used. Use unit specific manual as a guide
 - Unit Specific Check list
 - Design and overview of the DT Go unit
 - Insert O-rings where required
 - O-ring location and condition
 - Absorbent canister
 - Breathing loop
 - Automatic Diluent Valve: automatic and manual use
 - Manufacturer's supported add-ons: BOV, etc
2. Loop volume - minimum / optimum
 - Determine the correct counterlung size, & understand how to attain and maintain proper loop volume
3. Gas Physiology
 - Oxygen risks, Hypoxia, Hyperoxia
 - Carbon dioxide (CO₂) toxicity, Hypercapnia
 - Nitrogen absorption
4. Proper scrubber filling; in accordance with DT Go recommendations
 - Manufacturer's recommended scrubber medium, & procedures according to DT Go user manual
5. Electronic or Manual or Mechanical Systems Design and Maintenance
 - Oxygen (O₂) metabolizing calculations
 - Oxygen Sensors, limitations, care and replacement regime
 - System electronics functionality and calibration procedures
 - DT Go manual gas addition valve design and function. (raising and lowering of constant flow; determining correct flow rate for each individual)
6. Dive Tables
 - Constant partial pressure of oxygen (PPO₂) theory
 - Central nervous system (CNS) and Oxygen Tolerance Unit (OTU) tracking and awareness
7. Dive Computers
 - Mix adjustable
 - Constant PO₂
 - Decompression conservatism / Gradient factor selection
 - Oxygen (O₂) integrated

8. Dive Planning
 - Operational planning
 - Gas consumption
 - Scrubber duration
 - Gas requirements including bailout scenarios
 - Oxygen limitations
 - Nitrogen limitations
9. Emergency Procedures
 - Flooded loop
 - Cell warnings
 - Battery warnings
 - Electronic failures

Skills

1. Pre-dive checks
 - Specific Unit Checklist
 - Verify diluent and oxygen (O₂) cylinder contents using gas analyzers
 - Unit build-up
 - Scrubber canister filling
 - Breathing loop check including mouthpiece one-way valves and positive and negative check
 - Sensor calibration in oxygen, with verification in air
 - 5 minute pre-breathe
 - Bailout bottle/stage cylinder rigging
2. Demonstrate correct pre-dive planning procedures including
 - Limits based on system performance
 - Limits based on oxygen exposures at chosen PO₂ levels
 - Limits based on nitrogen absorption at planned depth and PO₂ set point
 - Appropriate selection of decompression conservatism / gradient factors for the planned dive
 - Thermal constraints
3. Underwater verification
 - Stop at 3-6 meters/9-19 feet on descent for leak bubble check
 - Counterlung & Over Pressure Valve adjustment, if necessary
4. Mouthpiece familiarity skills
 - BOV: switch between open and closed circuit
 - DSV: switch to bailout system
5. Adding diluent gas/ADV familiarity skills
 - ADV: Adding diluent gas and understand how it works
 - BOV: Use BOV to add diluent gas to the loop – 2 ways
 - Bail out second stage: Use to add diluent gas to the loop
 - Dual button MAV: Adding diluent gas (if unit is shipped with this item)
6. Emergency procedures: demonstrate appropriate response to the following; each dive should have a minimum of 2 “diver emergencies” that the student must react to.

- Practical bailout skills: including 2 open circuit ascents from approximately 18 meter/59 feet.
 - Gas shutdowns and loss of gas
 - Broken hoses
 - Flooded absorbent canister
 - Carbon dioxide (CO₂) breakthrough
 - Low oxygen drills
 - High oxygen drills
 - Flooding loop
 - Electronics, sensor, and battery failure
7. Practice transferring to open circuit bailout
 8. Rescue skill session as outlined by the training agency
 9. Use of a buoyancy control system
 - Buoyancy/trim control during dive
 - Buoyancy/trim control at safety stop
 10. Controlling and monitoring for PPO2 levels:
 - Raising/lowering PPO2
 - Starting PPO2
 - PPO2 monitoring every minute
 - Manual Add Valve verification: static at constant depth, monitor change over several minutes
 - Electronics systems monitoring for PPO2 levels (SETPOINT) and setpoint switching using manual and pre-programmed methods when available (when the unit is equipped with an on board decompression computer that monitors sensors)
 11. Electronic systems use:
 - Use and adjustment of Heads Up Display, position, brightness, colour
 - Use and adjustment of PPO2/depth/time display, position, brightness, colour
 - Use and adjustment of decompression computer, set up/gas switching, battery verification, etc
 12. Use of lift bag / DSMB and reel (where relevant and applicable)
 13. Mask removal and replacement
 14. Proper execution of the dive within all pre-determined dive limits
 15. Demonstration of safety stops at pre-determined depths (on all dives)
 16. Constant loop volume management
 17. Cell validation checks with appropriate use of diluent and oxygen
 - Oxygen sensor verification at depth
 - Do voltage limited test on sensors at approximately 5 meter/16 feet on pure oxygen
 18. Post dive clean of unit
 - Mouth piece and hoses
 - Clean and disinfect unit
 - Inspect components of unit
 19. Diver maintenance of unit

- Cell removal and replacement
- Mouthpiece care
- Replacing or re-charging of batteries

EXTRA REQUIREMENTS FOR COMPLETION

- Demonstrate an adequate level of fitness by completing a minimum of a 50m/164 feet surface diver tow with both the rescuer and the victim wearing a complete CCR diving system and bailout cylinder(s) applicable to their specific program.
- Complete all academic sessions and unit specific assessments as specified in the training material of the Training Agency and the Manufacturer.
- Complete a minimum of seven (7) training dives, including confined water skill development of at least one (1) hour, and six (6) core open water training dives with a minimum run time of 30 minutes each.
- Complete at least a minimum of 420 minutes of total in-water time on the applicable CCR unit.
- Be able to independently complete a full dive plan
- Complete a final course exam as set out by the training agency and / or manufacturer with a required minimum pass rate of 80% with 100% remediation.
- When the feature is available on a rebreather, download the student's dive logs of all training dives and retain for a minimum of seven years.
- If the feature is not available on a rebreather, download the dive logs from the students dive computer and retain for a minimum of seven years
- Fill in and sign a course completion form confirming all academics and practical sessions have been completed

Dive logs and student-signed course completion form are to be submitted to the manufacturer of the specific unit on request

DEPTH LIMITATIONS

- Open Water Training Dives shall be initially shallow, progressively increasing in depth.
- Two (2) dives must be deeper than 20 meters/65 feet for certification
- All dives must be conducted at a depth shallower than 30 meters/98 feet.

NOTES

- All training dives must be planned within the no-decompression limits of the Combined Air/EAN Tables or the student's personal dive computer or computer-generated decompression profiles.
- Bailout cylinder gas is to be based on a maximum PPO₂ of 1.6 at the maximum depth of the dive.
- Divers should not carry an on-board diluent gas with a PPO₂ higher than 1.1 bar at the bottom.
- The maximum loop set point is 1.3 bar.
- It is recommended that the student finish the training course within 6 weeks of the starting date.
- It is recommended that the student have access to, or purchase a unit within 3 months of completing the training program.
- Only approved training agencies and instructors may teach a DT Go rebreather course.

Diving in an overhead environment

This course shall not be conducted in an overhead environment. Subject to training agency approval certain dive sites can be deemed suitable for the CCR Diver course under the following conditions:

- The student must remain in the daylight zone where there is no need for the use of a dive light
- The student must never be a distance of more than 132 linear feet / 40 linear meters from the surface

SEQUENCE

Open Water Training Dives 1 and 2 may only be conducted after completing the equipment configuration section, the surface diver tow and all confined water sessions.

CERTIFICATION

The unit specific CCR Diver certification entitles the holder to dive with a buddy, diving on a rebreather or diving open circuit, utilizing CCR diving procedures to make non decompression dives to depths of up to 30 meters/98 feet, providing that dives are conducted in environments similar to those of the diver's training and experience.

CCR DIVER CROSSOVER

INTENT

The intent of the program is to provide divers already certified on a unit with additional unit specific training to get certified on an additional unit, following RESA minimum training standards.

REQUIRED INSTRUCTOR RATING

An active status unit specific CCR instructor at the level the candidate is crossing over for

ADMINISTRATIVE REQUIREMENTS

- Course liability release and assumption of risk (in accordance with local laws)
- Health screening document
- Anything else as required by the Training Agency or manufacturer

STUDENT PREREQUISITES

- Be certified as a CCR Diver from a RESA recognized training agency
- Show proof of 10 logged CCR dives in the last 12 months
- Minimum age 18 years

NOTE

- Crossover is not allowed for certifications on SCR or PSCR, or for CCR certifications that only allow a lesser dive depth: in all these cases a full course is mandatory
- Crossover applies to rebreathers of different brand/manufacturers
- Crossovers between similar units of the same brand/manufacturer may require an upgrade course as specified by the manufacturer

MATERIALS AND EQUIPMENT

- As specified in the specific diver level course standard

DURATION

- Recommended hours for course completion: 16 to 24
- The number of classes, hours and sessions per day are set by the training agency.

REQUIREMENTS FOR COMPLETION

The crossover course will include:

- CCR assembly workshop.
- A 60 minute water skills evaluation in a confined skill session. All skills from the level the candidate is crossing over at must be demonstrated successfully prior to open water dives.
- Complete a minimum of 4 open water dives and a total accumulated dive time of minimum 240 minutes, demonstrating proficiency in all skills from the level the diver is crossing over at
- Complete a final exam with a passing score as specified by the Training Agency and the Manufacturer.